



MAINTENANCE TRACKING TOOL

PETTRACE800



Date:2023-11-09

Country: Italy	Site: VEN
Intervention:	Single intervention <input checked="" type="checkbox"/>
Subsystems:	Vacuum <input checked="" type="checkbox"/>

VACUUM

Vacuum MFC curve test

SCCM	Chamber pressure	Backing pressure
1	0.00E+0	0.00E+0
2	5.70E-6	2.50E-2
3	0.00E+0	3.10E-2
4	1.20E-5	3.70E-2
5	1.50E-5	4.20E-2
6	1.70E-5	4.70E-2
7	1.80E-2	5.30E-2
8	2.00E-5	5.80E-2
9	2.30E-5	6.30E-2
10	2.50E-5	6.90E-2

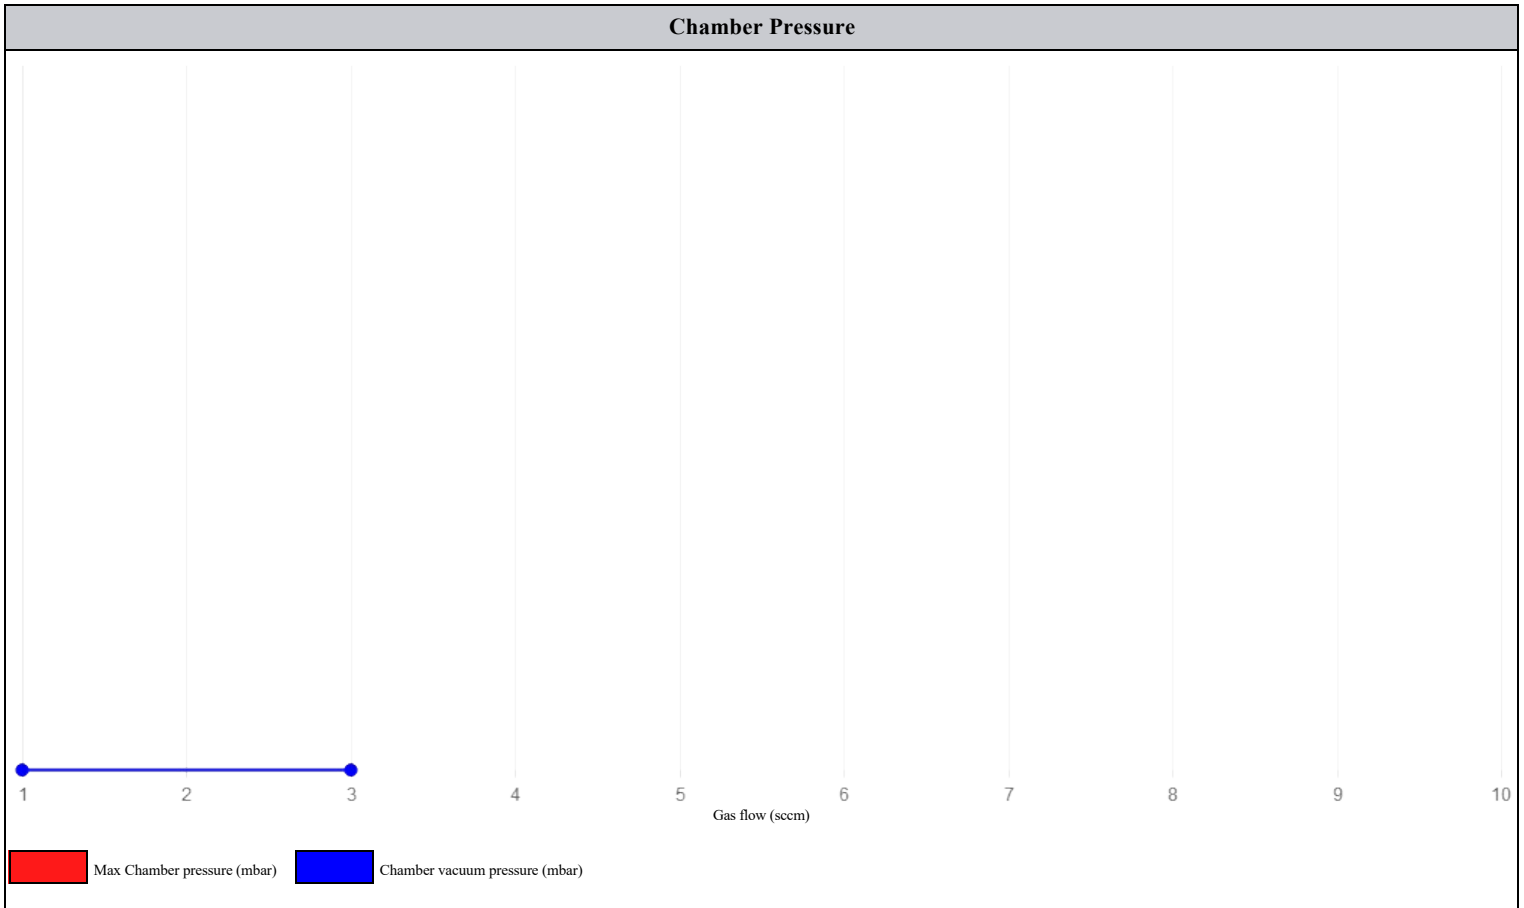

PETtrace800 O-Rings analysis

Pins

